



Instruction Sheet Whale 1080

Store these instructions in a safe place or with the enclosed maintenance checklist



Take time to familiarize yourself with the use and maintenance of this equipment before using. Please file this Instruction Sheet in an accessible location: the Instruction Sheet must be read and familiar to anyone who is using Southpaw Enterprises Equipment.

IMPORTANT: Please check equipment immediately for any damage that may have resulted during shipping. If any damage has occurred, please contact Southpaw Enterprises, Inc. immediately.

MATERIALS LIST

- | | |
|--------------------------|---|
| 1 - Whale | Vertical Stimulation Device Instruction Sheet |
| 4 - Double VSD Loops | Safety Snap Instruction Sheet |
| 4 - Locking Safety Snaps | Maintenance Checklist |
| 1 - Instruction Sheet | |

The Southpaw Whale can be used with the Southpaw Custom Support Structure and Upright Attachment Kit # 7030 (if your Custom Support Structure was ordered prior to October 1 st 2006) or two secure points at least 9 ft. apart and at least 36 in. above the floor.

Note: Each attachment point must be capable of holding the full working load of the Whale which is 300 lbs.

INSTRUCTIONS FOR USE

- The Whale is fully assembled, ready to connect to the attachment points. You may need to adjust the number of VSD loops to suit the weight of the client.
- Attach the VSD loops to the anchor point using the Safety Snap (See fig. 1). Take up the slack in the web strap on each end by grasping the tag end of the web strap and pulling on it while grasping the web strap on the other side of the buckle and pulling toward the buckle (See fig. 2). Be sure that the Whale is centered between the anchor points.
- Be sure that the attachment points are high enough that the client does not hit the floor.

Note: You may need to purchase additional VSD loops to accommodate the weight of heavier or multiple clients.

MATTING PRECAUTIONS: Always use appropriate mats under and around activity area.

WORKING LOAD: 300 lbs.

fig. 1


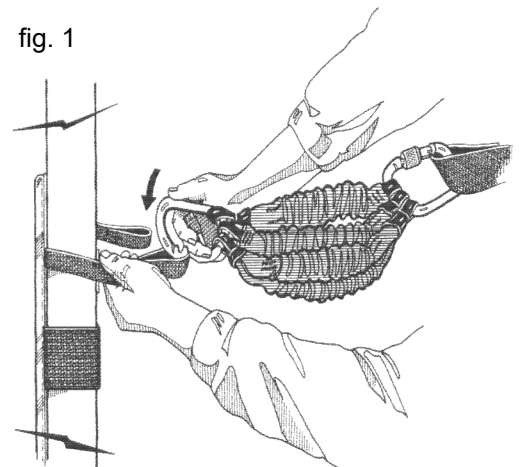


fig. 2

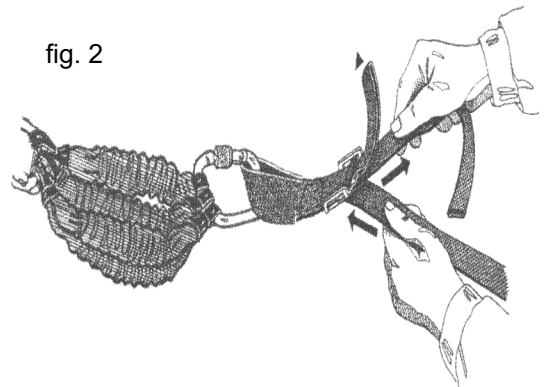

MAINTENANCE CHECKLIST:

All of the following wear points should be checked on a monthly basis and recorded on the checklist enclosed.

- Check the cover for loose stitches or torn seams. If loose stitches or tears are found, discontinue use until repaired.
- Check for excessive wear or fraying where web straps contact Safety Snaps. If excessive wear or fraying is found, discontinue use until repaired.
- Consult Vertical Stimulation Device Instruction Sheet for Maintenance Checklist for VSD.

STORAGE PROCEDURES

- Store out of direct sunlight.
- Store where not accessible by clients without proper supervision.

CLEANING INSTRUCTIONS

- Check with your infectious disease department before using these procedures.
- Check for client allergies first.
- Wipe vinyl with a damp cloth using soap and water of disinfectant.
- Dry before using.

Safety Precautions - The safety of your clients is dependent on the appropriate choice of activity to match, yet challenge their physical abilities. Use appropriate spotting / safety techniques. In addition, the layout of your activity area, proper installation and maintenance of your equipment is critical. Southpaw equipment is not intended for recreational or outdoor use. Under no condition should this equipment be used without proper supervision.

This sheet is for example only. It is not meant to, in any way, replace local, county, state, or Federal standards. Be aware - it is your responsibility to find all pertinent safety information that pertains to your facility.

If you have any questions or comments, please call or write

Southpaw Enterprises, Inc.

P.O. Box 1047, Dayton, Ohio 45401-1047

Toll Free - (800) 228-1698

Please visit us at southpaw.com

© 2020 Southpaw Enterprises, Inc.